TRILLIANT




ARSENAL FOOT PLATING SYSTEM™

The Arsenal Foot Plating System arms surgeons with variable angle locking technology and dual lead screws, a powerful combination of patented and innovative technologies, to address all types of fusions, fractures, and osteotomies in the forefoot, midfoot and rearfoot. This titanium alloy plating system offers a full "arsenal" for an extensive range of applications.

PLATING SYSTEMS




PLATE OFFERINGS

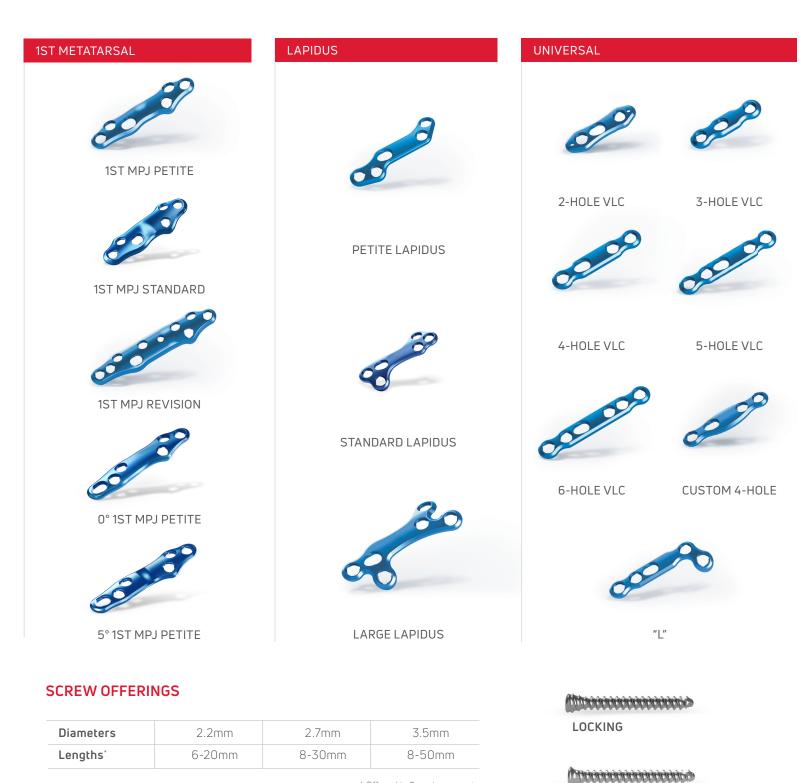

* Offered in 2mm increments

NON-LOCKING



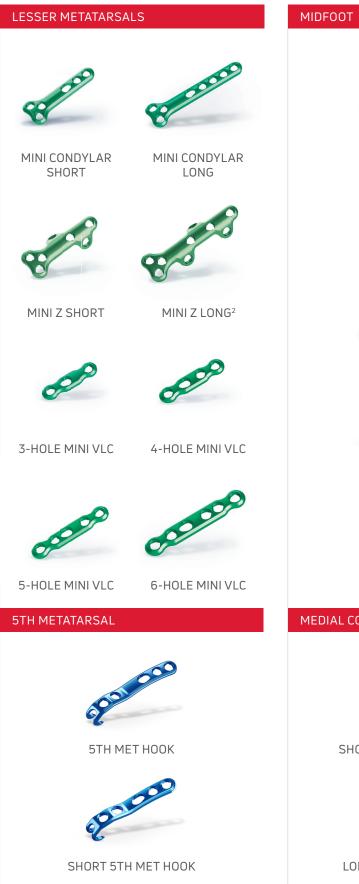

LISFRANC TN FUSION NC FUSION SMALL "U" STANDARD "U" MEDIAL COLUMN SHORT MEDIAL COLUMN

LONG MEDIAL COLUMN

REARFOOT/CALCANEAL



EVANS



CALCANEAL SLIDE



SINUS TARSI SUPPORT




PERIMETER



SINUS TARSI

TECHNOLOGY & FEATURES



CONE OF ANGULATION 60° Variable Angle, 20-50° more than the competition¹



DUAL-LEAD SCREWS Dual-lead screws seat up to 100% faster than single lead screws¹



MULTI-LOCK FUNCTIONALITY Repeatable, Locking & Relocking, Screw/Plate Interface




VANISHING EDGE PLATES Designed for minimal post-operative palpability without sacrificing strength


WHOLE FOOT SOLUTIONS



UNSURPASSED TECHNOLOGY



ANGLED 2.7MM LOCKING SCREW AVERAGE DISENGAGEMENT MOMENT¹



TURNS TO FULLY INSERT 2.7 X 18MM SCREW1



Competitor Screw C

Number of Turns 0 2 4 6 8 10 12 14 16 18 20

¹Data on file. ²Patent pending. Certain system features covered under U.S. Patent No. 10,743,922. FDA cleared 510(k) K191009. Trilliant products are made in the U.S.A.



T 800.495.2919 F 877.778.3864 727 North Shepherd Drive, Suite 100 I Houston, TX 77007 I U.S.A. djoglobal.com/foot-and-ankle

Copyright © 2021 by DJO, LLC 900-00-112 Rev F

Individual results may vary. DJO, LLC is a manufacturer of orthopedic implants and does not practice medicine. Only an orthopedic, or foot and ankle surgeon can determine what treatment is appropriate. The contents of this document do not constitute medical, legal, or any other type of professional advice. This material is intended for the sole use and benefit of the DJO, LLC sales force and physicians. It is not to be redistributed, duplicated, or disclosed without the express written consent of DJO, LLC. For more information on risks, warnings, and possible adverse side effects refer to the Instructions for Use provided with the device

